



Please read this manual before operating

# UDS-L LED ULTRASONIC SCALER

## INSTRUCTION MANUAL



[www.glwoodpecker.com](http://www.glwoodpecker.com)

**GUILIN WOODPECKER MEDICAL INSTRUMENT CO., LTD.**

## Contents

1. The installation and components of equipment .....	1
2. Product function and operation .....	5
3. Maintenance .....	8
4. Cleaning, Disinfection and Sterilization .....	10
5. Precaution .....	16
6. After service .....	17
7. Symbol instruction .....	18
8. Environmental protection .....	18
9. Manufacturer's right .....	18
10. European authorized representative .....	19
11. EMC-Declaration of conformity .....	19
12. Statement .....	22
TABLE OF OPERATING POWER OF THE TIPS.....	23

## **1. The installation and components of equipment**

### 1.1 Instruction

Guilin Woodpecker Medical Instrument Co., Ltd. is a professional manufacturer in researching, developing and producing ultrasonic scalers. The product is mainly used for teeth cleaning and also an indispensable equipment for teeth disease prevention and treatment. The new product UDS-L LED ultrasonic scaler has scaling, perio, automatic water supply system (optional) and endo functions. It contains the following features:

1.1.1 Optical handpiece, more convenient for clinical operation.

1.1.2 Automatic frequency tracking ensures that the machine always works on the best frequency and performs more steadily. The optional function: automatic water supply system.

1.1.3 The handpiece is detachable and can be autoclaved to the high temperature of 134°C and pressure of 0.22MPa.

1.1.4 Digital controlled, easy operation and more efficient for scaling.

These features make UDS-L LED to be the new generation product in world dental market.

### 1.2 Components

1.2.1 The components of the machine are listed in the packing list.

1.2.2 Product performance and structure

Ultrasonic scaler is composed of electrocircuit, water way and ultrasonic transducer.

1.2.3 Scope of application

Ultrasonic scaler UDS-L LED is used for the dental calculus elimination and root canal treatment.

### 1.3 The main technical specifications

1.3.1 Technical specifications of ultrasonic scaler

a) Power supply input: 220-240V~ 50Hz/60Hz 150mA

b) Main unit input: 24V~ 50Hz/60Hz 1.3A  
5V~ 50Hz/60Hz 200mA (optional)

c) Output primary tip Vibration excursion :  $\leq 100\mu\text{m}$

d) Output half-excursion force :  $< 2\text{N}$

e) Output tip vibration frequency: 28kHz $\pm$ 3kHz

f) Output power: 3W to 20W

g) Main unit fuse: 250VT 1.6AL

h) Power supply fuse: 250VT 0.5AL

- i) Water pressure: 0.1bar to 5bar (0.01MPa to 0.5MPa)
- j) Weight of main unit: 0.73kg
- k) Weight of power supply: 1 kg
- l) Operating mode: Continuous operation
- m) Type of protection against electric shock: Class II equipment
- n) Degree of protection against electric shock: Type BF applied part
- o) Applied part of the equipment: handpiece and tip
- p) Degree of protection against harmful ingress of water: Ordinary equipment
- q) Protection degree against water(used on the pedal): IPX1
- r) Degree of safety of application in the presence of a Flammable Anaesthetic Mixture with air or with Oxygen or Nitrous Oxide Equipment not suitable for being used in the presence of a flammable anaesthetic mixture with air or with oxygen or nitrous oxide.


### 1.3.2 Working condition


- a) Environment temperature: +5°C to +40°C
- b) Relative humidity: 30% ~75%
- c) Atmosphere pressure: 70kPa to 106kPa
- d) A temperature of the water at the inlet: not higher than +25°C

## 1.4 Installation of the main components

### 1.4.1 Sketch map for installation and connection.


- a) Sketch map for front panel and back panel of main unit are showed in picture1

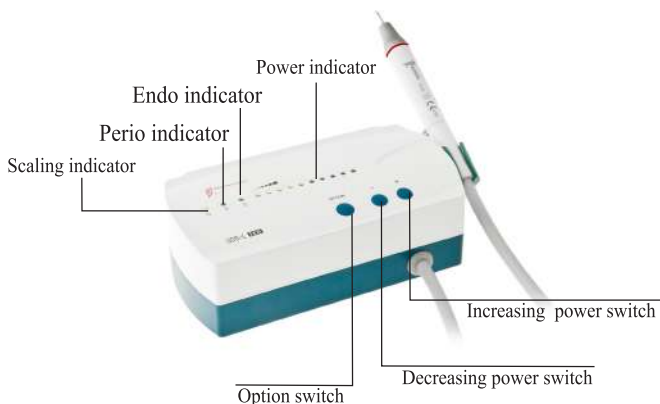

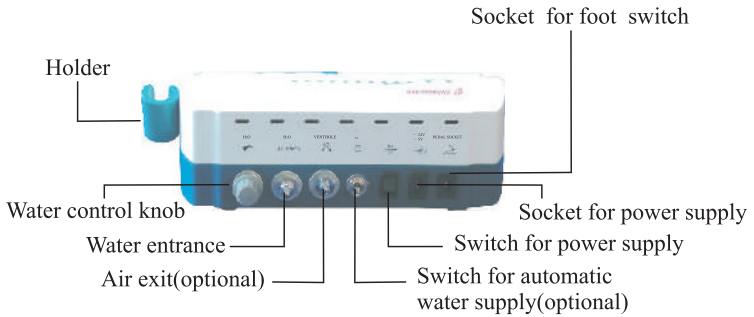


picture1

b) Sketch map for connection of foot switch, power supply and main unit are showed in picture2

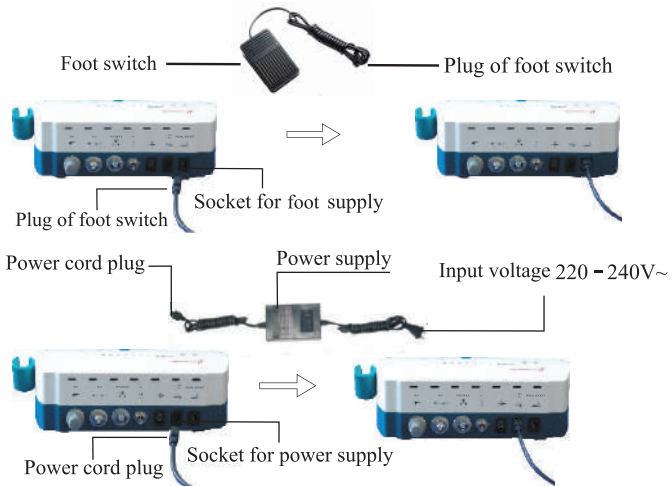


picture2

c) Sketch map for connection of water supply system are showed in picture3

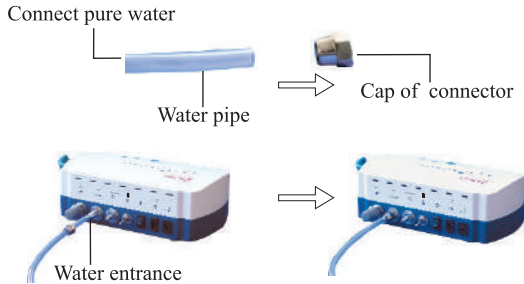


picture3

d) Sketch map for automatic water supply system (optional) are showed in picture4

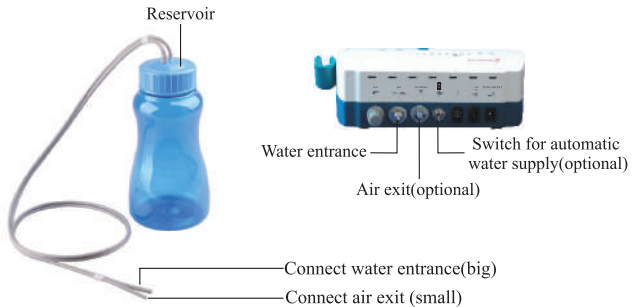


picture4

e) Sketch map for connection of detachable handpiece are showed in picture5

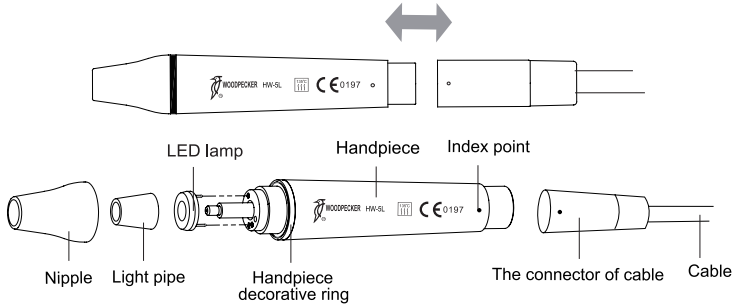

picture5

f) Sketch map for how to install tip and endochuck with wrench are showed in picture6

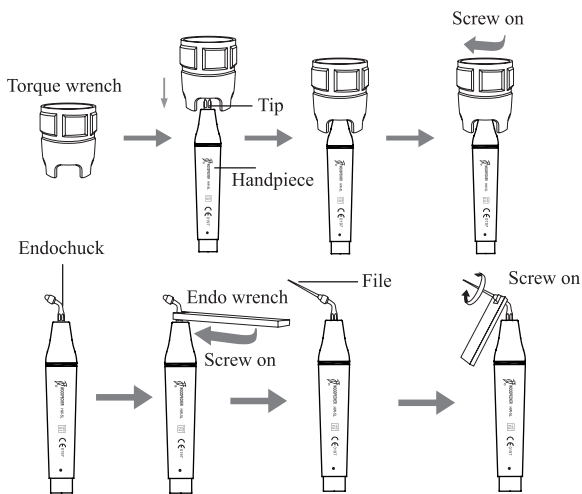

picture 6

## 2. Product function and operation

### 2.1 Scaling function

#### 2.1.1 Operation

a) Open the packing box, make sure that all the parts and accessories are complete according to the packing list. Take the main unit out of the box and put it on a stable plane.

b) Turn the water control knob to the max based on symbol as shown as 3.5.2 [note 1].

c) Insert the plug of the foot switch to its socket (picture 2).

d) Connect one end of the water pipe to the water entrance, and the other end to the clean water source (picture 3).

e) Screw the scaling tip tightly to handpiece by torque wrench , then connect the handpiece and the connector of cable correctly.

f) Connect the main unit with output plug of power supply, then connect to the power (picture 2).

g) Switch on the main unit, then the scaling indicator and the first five lead lights of power indicator shine.

h) Select a suitable scaling tip as you need, screw it on the handpiece tightly by the torque wrench (picture 6).

i) Step on the foot switch, the tip begins to vibrate, and the LED lamp on the top of the handpiece shines. Release the foot switch, the LED lamp keep shining for 10 seconds.

j) The normal frequency is extremely high. Under the normal working state

of the scaling tip, a light touch and a certain to-and-fro motion will eliminate the tartar without heating. Overexertion and long-time lingering are forbidden.

k) Vibrating intensity: Adjust the vibration intensity as you need, generally turn the knob to the middle grade. According to patient's different sensitivity and the rigidity of the gingival tartar, adjust the vibration intensity during the clinical treatment.

l) Water volume adjustment: Step on the foot switch, and the tip begins to vibrate, then turn the water control knob to form fine spray to cool down the handpiece and clean the teeth.

m) The handpiece can be handled in the same gesture as a pen in hand.

n) During the clinical treatment, be sure not to make the end of tip touch the teeth vertically and not to make the tip overexert on the surface of the teeth in case of hurting the teeth and damaging the tip.

o) After finishing operation, keep the machine working for 30 seconds on the water supply condition in order to clean the handpiece and the scaling tip.

p) Unscrew the scaling tip and pull out handpiece, then sterilize them.

**Notice: Don't pull out the handpiece when the foot switch is stepped on and the machine is working.**

2.1.2 Instruction for main components of detachable handpiece (showed in picture 5):

a) Nipple: The nipple can be removed. You can screw off the nipple and clean the pole with alcohol termly.

b) Decorative ring: can be disassembled and cleaned with alcohol regularly, can be autoclaved under the high temperature and pressure.

c) Handpiece: The main part of the whole handpiece, can be autoclaved under the high temperature and pressure.

d) The connector of the cable: Connect the handpiece with the water source and power supply of the main unit.

e) LED lamp、Light pipe: Clean them with purified water and sterilize them under the high temperature of 134°C and high pressure of 0.22Mpa.

**Notice: Keep the joint of handpiece and the cable connector dry.**

2.1.3 Instruction of using torque wrench (showed in picture 6)

a) The torque wrench's structure is designed in special way which can control the strength of the scaling tip's installation properly and correctly. It also can guarantee the operator screw or unscrew the scaling tip effectively and keep their hands away from being scratched.

b) Operation

① Take the scaling tip into the torque wrench, operate as showed in picture 6.

② Tip installation: Hold the handpiece, turn the tip toward direction as showed in picture 6 with the torque wrench. Turn one more circles when the tip stops, then the tip is installed.



③ Tip uninstallation: Hold the handpiece, turn the wrench toward anti-clockwise direction.

④ Sterilize it in sterilizer after each treatment.

⑤ The torque wrench must be cooled naturally after sterilization to avoid scalding when using next time.

⑥ Keep the torque wrench in a cool, dry and ventilated place and keep it clean.

#### 2.1.4 Automatic water supply system (optional)

##### a) Usage process

① After adding enough water into the reservoir, install the reservoir cap on the reservoir properly and tighten it up.

② The twin tube is composed of two pipes. The big one is water pipe, and small one is air pipe. Connect the small one to AIR connector on the reservoir, connect the big one to H<sub>2</sub>O connector.

③ Turn on the automatic water supply switch on the main unit.

##### b) Precaution

① Please operate correctly according to the manual, the reservoir cap must be tightened up.

② When adding or changing water, please pull out the air pipe first, then pull out the water pipe.

③ Under normal automatic water supply condition, the air pump produces the "WOO" sound intermittently, which is common phenomenon.

## 2.2 Endo function

### 2.2.1 Usage process

a) Fix endochuck to handpiece by endo wrench. (See picture 6)

b) Unscrew the screw cap on the endochuck.

c) Put the ultrasonic file into the hole in the front of endochuck.

d) Screw down the screw cap with endo wrench, to tight up the ultrasonic file.

e) Press option key, turn to endo function, then the indicator of endo function is on.

f) When ultrasonic scaler turns into endo function, only the first lead light is on and the power is at the first grade. Put the ultrasonic file into the patient's root canal slowly, step on the foot switch, then make endo treatment. During the treatment, turn up the power gradually according to the needs.

### 2.2.2 Notice

**a) When fixing endochuck, it must be screwed down.**

**b) The screw cap on the endochuck must be screwed down.**

**c) Don't press it too hard when the ultrasonic file is in the root canal.**

**d) Don't step on the foot switch until the ultrasonic file is in the root canal. The power range is supposed from the 1st to 5th grade.**

### 3. Maintenance

#### 3.1 Troubleshooting

Fault	Possible	Solutions
The scaling tip doesn't vibrate and there is no water flowing out when stepping on the foot switch.	The power plug is in loose connect.	Make the plug insert to the socket well
	The foot switch is in loose contact.	Insert the foot switch to its socket tightly.
	The fuse of transformer is broken	Contact our dealers or us.
	The fuse in the main unit is broken	Contact our dealers or us.
The scaling tip doesn't vibrate but there is water flowing out when stepping on the foot switch.	The tip is in loose contact.	Screw the tip on the handpiece tightly (picture 6).
The scaling tip vibrates but there is no spray when stepping on the switch.	The connect plug between the handpiece and the circuit board is in loose contact.	Contact our dealers or us.
	Something wrong with the handpiece.	Send it to our company to repair.
	Something wrong with the cable.	Contact our dealers or us.
	The water control switch is not on.	Turn on the water control switch [note 1].
	There is impurity in the solenoid valve.	Contact our dealers or us.
	The water system is blocked.	Clean the water line by multi-function syringe [note 2].

Fault	Possible	Solutions
There is still water flowing out after the power is off.	There is impurity in the solenoid valve.	Contact our dealers or us.
The handpiece generates heat.	The water control switch is in a low setting.	Turn the water control switch to a higher grade [note 2].
The amount of spouting water is too little.	The water pressure is not high enough.	Make the water pressure higher.
	The water line is blocked.	Clean the water pipe by multi-function syringe [note 2].
The vibration of the tip becomes weak.	The tip hasn't been screwed on to the handpiece tightly.	Screw the tip on the handpiece tightly(as showed in picture 6).
The vibration of the tip becomes weak.	The tip is loose because of vibration.	Screw on the tip tightly (as showed in picture 6).
	The joint of the handpiece and the cable isn't dry.	Dry it by the hot air.
	The tip is damaged [note 3]	Change a new one.
There is water seeping from the joint of the handpiece and the cable.	The waterproof "O" ring is damaged.	Change a new "O" ring.
The u-file doesn't vibrate.	The screw cap is loose.	Tighten it.
	Endochuck is damaged.	Change a new one.
LED light don't work	Poor contact	Contact tightly
	Something wrong with LED light	Change a new one
	LED lamp installed backwards	Please install the "+" of the LED lamp to the "+" of the handpiece

Fault	Possible	Solutions
There is noise coming from the endochuck	The screw cap is loose.	Tighten it.

If the problem still can't be solved, please contact with local dealer or manufacturer.

### 3.2 Notice

[Note 1] The water control knob can adjust the water volume according to the symbol

[Note 2] Clean the water pipe with the multi-function syringe of the dental unit (as showed in picture 7)



picture7

- Cut the water pipe at a distance of 10cm~20cm from the water entrance.
- Turn on the power switch.
- Connect the multi-function syringe of dental unit to the water pipe.
- Disassemble the tip or handpiece.
- Step on the foot switch.
- Turn on the switch of the multi-function syringe, press the water into the machine and the impurity blocked in the water pipe can be eliminated.

[Note 3] If the scaling tip has been screwed on tightly and there is fine spray too, the following phenomena show that the scaling tip is damaged:

- The vibrating intensity and the water atomization degree become weak obviously.
- During treatment, it produces the sound like "buzz" from the scaling tip.

## 4. Cleaning, Disinfection and Sterilization

The cleaning, disinfection and sterilization of handpiece, tip, and wrench (include torque wrench and Endo wrench) are as follow.

Unless otherwise stated, they will be hereinafter referred to as "products".

### Warnings

The use of strong detergent and disinfectant (alkaline pH>9 or acid pH <5) will reduce the life span of products. And in such cases, the manufacturer takes no responsibility.

Do not clean the handpiece with ultrasound cleaning machine.  
This device shall not be exposed to high temperature above 138°C.

### **Processing limit**

The products have been designed for a large number of sterilization cycles. The materials used in manufacture were selected accordingly. However with every renewed preparation for use, thermal and chemical stresses will result in ageing of the products. The maximum number of sterilizations for handpiece is 600 times. For tips, it is 300 times. And for wrench, it is 1000 times.

## 4.1 Initial processing

### 4.1.1 Processing principles

It is only possible to carry out effective sterilization after the completion of effective cleaning and disinfection. Please ensure that, as part of your responsibility for the sterility of products during use, only sufficiently validated equipment and product-specific procedures are used for cleaning/disinfection and sterilization, and that the validated parameters are adhered to during every cycle.

Please also observe the applicable legal requirements in your country as well as the hygiene regulations of the hospital or clinic, especially with regard to the additional requirements for the inactivation of prions.

### 4.1.2 Post-operative treatment

The post-operative treatment must be carried out immediately, no later than 30 minutes after the completion of the operation. The steps are as follows:

1. Let the Ultrasonic Scaler works for 20-30 seconds at maximum water volume to flush the handpiece and tip;
2. Remove the handpiece from the Ultrasonic scaler, and rinse away the dirt on the surface of product with pure water (or distilled water/deionized water);
3. Dry the product with a clean, soft cloth and place it in a clean tray.

Notes

- a) The water used here must be pure water, distilled water or deionized water.

## 4.2 Preparation before cleaning

Steps


Tools: Torque wrench, tray, soft brush, clean and dry soft cloth.

1. Remove the tip from product with torque wrench provided by Guilin Woodpecker Medical Instrument Co., Ltd, and then put the tip and wrench into a clean tray.

2. Unscrew the nipple of product counterclockwise, remove the sealing ring, light pipe (if any), and LED lamp(if any), and put them in the tray.

3. Use a clean soft brush to carefully brush the joints between product and the connector of cable, front thread, horn, nipple, seal ring, light pipe(if any) and LED lamp(if any) until the dirt on surface is not visible. Then use soft cloth to dry the product and accessories and put them into a clean tray. The cleaning agent can be pure water, distilled water or deionized water.

## Disassembling steps

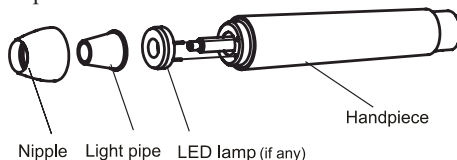

### 4.3 Cleaning

The cleaning should be performed no later than 24 hours after the operation.

The cleaning can be divided into automated cleaning and manual cleaning. Automated cleaning is preferred if conditions permit.

#### 4.3.1 Automated cleaning

- The cleaner is proved to be valid by CE certification in accordance with EN ISO 15883.

- There should be a flushing connector connected to the inner cavity of the product.

- The cleaning procedure is suitable for the product, and the irrigating period is sufficient.

- Do not clean the handpiece with ultrasound.

It is recommended to use a washer-disinfector in accordance with EN ISO 15883. For the specific procedure, please refer to the automated disinfection section in the next section “Disinfection”.

#### Notes

a) The cleaning agent does not have to be pure water. It can be distilled water, deionized water or multi-enzyme. But please ensure that the selected cleaning agent is compatible with the product.

b) In washing stage, the water temperature should not exceed 45 °C, otherwise the protein will solidify and it would be difficult to remove.

c) After cleaning, the chemical residue should be less than 10mg / L.

### 4.4 Disinfection

Disinfection must be performed no later than 2 hours after the cleaning phase. Automated disinfection is preferred if conditions permit.

#### 4.4.1 Automated disinfection-Washer-disinfector

- The washer-disinfector is proved to be valid by CE certification in accordance with EN ISO 15883.

- Use high temperature disinfection function. The temperature does not exceed 134 ° C, and the disinfection under the temperature cannot exceed 20 minutes.

- The disinfection cycle is in accordance with the disinfection cycle in EN ISO 15883.

Cleaning and disinfecting steps by using Washer-disinfector

1. Carefully place the product into the disinfection basket. Fixation of product is needed only when the product is removable in the device. The products are not

allowed to contact each other.

2. Use a suitable rinsing adaptor, and connect the internal water lines to the rinsing connection of the washer-disinfector.

3. Start the program.

4. After the program is finished, remove the product from the washer-disinfector, inspect (refer to section “Inspection and Maintenance”) and packaging (refer to chapter “Packaging”). Dry the product repeatedly if necessary (refer to section “Drying”).

#### Notes

a) Before use, you must carefully read the operating instructions provided by the equipment manufacturer to familiarize yourself with the disinfection process and precautions.

b) With this equipment, cleaning, disinfection and drying will be carried out together.

c) Cleaning: (c1) The cleaning procedure should be suitable for the product to be treated. The flushing period should be sufficient (5-10 minutes). Pre-wash for 3 minutes, wash for another 5 minutes, and rinse it for twice with each rinse lasting for 1 minute. (c2) In the washing stage, the water temperature should not exceed 45 °C, otherwise the protein will solidify and it is difficult to remove. (c3) The solution used can be pure water, distilled water, deionized water or multi-enzyme solution, etc., and only freshly prepared solutions can be used. (c4) During the use of cleaner, the concentration and time provided by manufacturer shall be obeyed. The used cleaner is neodisher MediZym (Dr. Weigert).

d) Disinfection: (d1) Direct use after disinfection: temperature  $\geq 90$  ° C, time  $\geq 5$  min or  $A0 \geq 3000$ .

(d2) Sterilize it after disinfection and use: temperature  $\geq 90$  ° C, time  $\geq 1$  min or  $A0 \geq 600$ .

(d3) For the disinfection here, the temperature is 93 ° C, the time is 2.5 min, and  $A0 > 3000$ .

e) Only distilled or deionized water with a small amount of microorganisms ( $< 10$  cfu/ml) can be used for all rinsing steps. (For example, pure water that is in accordance with the European Pharmacopoeia or the United States Pharmacopoeia).

f) After cleaning, the chemical residue should be less than 10mg / L.

g) The air used for drying must be filtered by HEPA.

h) Regularly repair and inspect the disinfector.

#### 4.5 Drying

If your cleaning and disinfection process does not have an automatic drying function, dry it after cleaning and disinfection.

##### Methods

1. Spread a clean white paper (white cloth) on the flat table, point the product against the white paper (white cloth), and then dry the product with filtered dry

compressed air (maximum pressure 3 bar). Until no liquid is sprayed onto the white paper (white cloth), the product drying is completed.

2. It can also be dried directly in a medical drying cabinet (or oven). The recommended drying temperature is 80°C~120°C and the time should be 15~40 minutes.

Notes

- a) The drying of product must be performed in a clean place.
- b) The drying temperature should not exceed 138 °C;
- c) The equipment used should be inspected and maintained regularly.

#### 4.6 Inspection and maintenance

In this chapter, we only check the appearance of the product. After inspection, if there is no problem, the handpiece should be immediately reassembled, installing the sealing ring, LED, light guide, and cone head in sequence to the handpiece, and then tighten the cone head clockwise.

4.6.1 Check the product. If there is still visible stain on the product after cleaning/disinfection, the entire cleaning/disinfection process must be repeated.

4.6.2 Check the product. If it is obviously damaged, smashed, detached, corroded or bent, it must be scrapped and not allowed to continue to be used.

4.6.3 Check the product. If the accessories are found to be damaged, please replace it before use. And the new accessories for replacement must be cleaned, disinfected and dried.

4.6.4 If the service time (number of times) of the product reaches the specified service life (number of times), please replace it in time.

#### 4.7 Packaging

Install the disinfected and dried product and quickly package it in a medical sterilization bag (or special holder, sterile box).

Notes

- a) The package used conforms to ISO 11607;
- b) It can withstand high temperature of 138 °C and has sufficient steam permeability;
- c) The packaging environment and related tools must be cleaned regularly to ensure cleanliness and prevent the introduction of contaminants;
- d) Avoid contact with parts of different metals when packaging.

#### 4.8 Sterilization

Use only the following steam sterilization procedures (fractional pre-vacuum procedure\*) for sterilization, and other sterilization procedures are prohibited:

- The steam sterilizer complies with EN13060 or is certified according to EN 285 to comply with EN ISO 17665;
- The highest sterilization temperature is 138 °C;
- The sterilization time is at least 4 minutes at a temperature of 132°C/134°C and a pressure of 2.0 bar ~ 2.3 bars.



- Allow a maximum sterilization time of 20 minutes at 134 °C.

Verification of the fundamental suitability of the products for effective steam sterilization was provided by a verified testing laboratory.

Notes

a) Only products that have been effectively cleaned and disinfected are allowed to be sterilized;

b) Before using the sterilizer for sterilization, read the Instruction Manual provided by the equipment manufacturer and follow the instructions.

c) Do not use hot air sterilization and radiation sterilization as this may result in damage to the product;

d) Please use the recommended sterilization procedures for sterilization. It is not recommended to sterilize with other sterilization procedures such as ethylene oxide, formaldehyde and low temperature plasma sterilization. The manufacturer assumes no responsibility for the procedures that have not been recommended. If you use the sterilization procedures that have not been recommended, please adhere to related effective standards and verify the suitability and effectiveness.

\* Fractional pre-vacuum procedure = steam sterilization with repetitive pre-vacuum. The procedure used here is to perform steam sterilization through three pre-vacuums.

#### 4.9 Storage

1. Store in a clean, dry, ventilated, non-corrosive atmosphere with a relative humidity of 10% to 93%, an atmospheric pressure of 70KPa to 106KPa, and a temperature of -20 °C to +55 °C;

2. After sterilization, the product should be packaged in a medical sterilization bag or a clean sealing container, and stored in a special storage cabinet. The storage time should not exceed 7 days. If it is exceeded, it should be reprocessed before use.

Notes:

a) The storage environment should be clean and must be disinfected regularly;

b) Product storage must be batched and marked and recorded.

#### 4.10 Transportation

1. Prevent excessive shock and vibration during transportation, and handle with care;

2. It should not be mixed with dangerous goods during transportation.

3. Avoid exposure to sun or rain or snow during transportation.

**The cleaning and disinfection of main unit are as follows.**

- Before each use, wipe the surface of the main unit, the connector of cable and cable with a soft cloth or paper towel soaked in 75% medical alcohol. Repeat the wipe for at least 3 times.

- Before each use, please let the Ultrasonic scaler works for 20-30 seconds at

maximum water volume, then install the handpiece.

- After each use, please let the Ultrasonic scaler works for 20-30 seconds at maximum water volume, then remove the handpiece.

- After each use, wipe the surface of the main unit, the connector of cable and cable with a soft cloth soaked in clean water (distilled or deionized water) or a clean disposable wipe. Repeat the wipe for at least 3 times.

## **5. Precaution**

### 5.1 Notice when using equipment

5.1.1 Keep the scaler clean before and after operation.

5.1.2 The handpiece, scaling tip, torque wrench, endo wrench and endochuck must be sterilized before each treatment.

5.1.3 Don't screw the scaling tip and endochuck when stepping on the foot switch.

5.1.4 The scaling tip must be fastened and there must be fine spray or drip coming out from the tip when operating.

5.1.5 Change a new one when the tip and ultrasonic file are damaged or worn excessively.

5.1.6 While scaler working ,the heat of scaling tip will become higher if there is no water flowing out.Please keep the water flow smoothly.

5.1.7 Don't twist or rub the tip and endochuck.

5.1.8 Don't use impure water source and be sure not use normal brine instead of pure water source.

5.1.9 If use the water source without hydraulic pressure, the water surface should be one meter higher than the head of the patient.

5.1.10 Keep the connector of handpiece and the socket of the cable dry before installing the handpiece.

5.1.11 Don't pull the cable forcibly in case of the handpiece falling off from the cable.

5.1.12 Don't knock or rub the handpiece.

5.1.13 Please put the power plug into the socket easy to pull out, to make sure it can be pulled out in emergency.

5.1.14 The power supply is considered as a part of ME equipment.The power supply is a part of the device. This device can only be equipped with the special power supply of Guilin Woodpecker Medical Instrument Co., Ltd.

5.1.15 The power supply is NOT waterproof. Please keep it dry and away from the water.

5.1.16 After operation, turn off the power, then pull out the plug.

5.1.17 We are only responsible for the safety on the following conditions

a) The maintenance, repair and modification are made by the manufacturer or the authorized dealer

a) The exchanged components are original of "WOODPECKER" and operated according to instruction manual.

5.1.18 The internal screw thread of the scaling tips produced by some manufacturers maybe coarse, rusty and collapsed. This will damage the external screw thread of the handpiece irretrievably. Please use "WOODPECKER" brand scaling tips.

5.1.19 Please select a suitable power when using different type of tips (refer to "TABLE OF OPERATING POWER OF THE TIPS").

## 5.2 Contraindication

5.2.1 The hemophilia disease patient is not allowed to use this equipment.

5.2.2 The patients or doctors with heart pacemaker are forbidden to use this equipment.

5.2.3 The heart disease patient, pregnant woman and children should be cautious to use the equipment.

## 5.3 Storage and maintenance

5.3.1 The equipment should be handled carefully and lightly. Be sure that it is far from the vibration, and installed or kept in a cool, dry and ventilated place.

5.3.2 Don't store the machine together with the articles that are combustible, poisonous, caustic or explosive.

5.3.3 This equipment should be stored in a room where the relative humidity is 10% ~ 93%, atmospheric pressure is 70kPa to 106kPa, and the temperature is -20°C ~ +55°C.

5.3.4 If the machine is not used for a long time, please make it get through the power and water once per month for five minutes.

## 5.4 Transportation

5.4.1 Excessive impact and shake should be prevented in transportation. Lay it carefully and lightly and don't invert it.

5.4.2 Don't put it together with dangerous goods during transportation.

5.4.3 Avoid solarization and getting wet in rain or snow during transportation.

## **6. After service**

We offer one year's free repair to the equipment according to the warranty card.

The repair of the equipment should be carried out by our professional technician

We are not responsible for any irretrievable damage caused by the non-professional person.

## 7. Symbol instruction




WOODPECKER Trademark

**IPX0** Ordinary equipment

 Alternating current

**IPX1** Drip-proof


 Date of manufacture

 Manufacturer


 Class II equipment


 Type BF applied part


 Foot switch interface


 Used indoor only

 Adjustment for the water flow

 Can be autoclaved

 Follow Instructions for Use


 Water entrance pressure  
0.01MPa-0.5MPa

 **0197** CE marked product

 Power switch


VENTHOLE


 Air exit


 Switch of automatic water supply

 ~24V  
 ~5V  
Connection of the electrical supply of 24V~, 5V~

 Appliance compliance WEEE directive

 Atmospheric pressure for storage  
108kPa  
78kPa

 Temperature limitation for storage  
155°C  
-20°C

 Humidity limitation for storage  
93%  
10%



Authorised Representative in the EUROPEAN COMMUNITY

## 8. Environmental protection

Please dispose according to the local laws.

## 9. Manufacturer's right

We reserve the right to change the design of the equipment, the technique, fittings, the instruction manual and the content of the original packing list at any

time without notice. If there are some differences between blueprint and real equipment, take the real equipment as the norm.

### 10. European authorized representative




MedNet EC-Rep GmbH  
Borkstrasse 10 · 48163 Muenster · Germany

### 11. EMC-Declaration of conformity

Guidance and manufacturer's declaration - electromagnetic emissions		
The model UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED are intended for use in the electromagnetic environment specified below. The customer or the user of the model UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED use RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR11	Class B	The models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED are suitable for used in domestic establishment and in establishment directly connected to a low voltage power supply network which supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Complies	

<b>Guidance &amp; Declaration — electromagnetic immunity</b>			
The models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED are intended for use in the electromagnetic environment specified below. The customer or the user of the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED should assure that It is used in such an environment.			
<b>Immunity test</b>	<b>IEC 60601 test level</b>	<b>Compliance level</b>	<b>Electromagnetic environment - guidance</b>
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electrical fast transient/burst IEC 61000-4-4	±2kV for power supply lines ±1 kV for Input/output lines	±2kV for power supply lines ±1kV for interconnecting cable	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV line to line ±2 kV line to earth	±1 kV line to line	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11.	<5 % $U_T$ (>95% dip in $U_T$ ) for 0.5 cycle 40 % $U_T$ (60% dip in $U_T$ ) for 5 cycles 70% $U_T$ (30% dip in $U_T$ ) for 25 cycles <5% $U_T$ (>95 % dip in $U_T$ ) for 5 sec	<5 % $U_T$ (>95% dip in $U_T$ ) for 0.5 cycle 40 % $U_T$ (60% dip in $U_T$ ) for 5 cycles 70% $U_T$ (30% dip in $U_T$ ) for 25 cycles <5% $U_T$ (>95 % dip in $U_T$ ) for 5 sec	Mains power quality should be that of a typical commercial or hospital environment. If the user of the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED require continued operation during power mains interruptions, it is recommended that the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE $U_T$ is the a.c. mains voltage prior to application of the test level.			

Guidance & Declaration - Electromagnetic immunity			
The models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED are intended for use in the electromagnetic environment specified below. The customer or the user of the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Conducted RF IEC 61000-4-6 Radiated RF IEC 61000-4-3	3 Vrms 150 kHz to 80 MHz 3 V/m 80 MHz to 2.5 GHz	3V 3 V/m	<p>Portable and mobile RF communications equipment should be used no closer to any part of the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p><b>Recommended separation distance</b></p> <p>3V</p> <p><math>d=1.2 \times P^{1/2}</math> 80 MHz to 800 MHz</p> <p><math>d=2.3 \times P</math> 800 MHz to 2.5 GHz</p> <p>where <math>P</math> is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and <math>d</math> is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,<sup>a</sup> should be less than the compliance level in each frequency range.<sup>b</sup></p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
NOTE 1 At 80 MHz end 800 MHz. the higher frequency range applies.			
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			
<sup>a</sup> Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED are used exceeds the applicable RF compliance level above, the model UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED.			
<sup>b</sup> Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3V/m.			

<b>Recommended separation distances between portable and mobile RF communications equipment and the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED</b>			
The model UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED is intended for use in electromagnetic environment in which radiated RF disturbances is controlled. The customer or the user of the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the models UDS-J, UDS-K, UDS-K LED, UDS-L, UDS-L LED, UDS-A, UDS-A LED, UDS-P, UDS-E, UDS-P LED, UDS-E LED, D1, D3, D5, D7, D3 LED, D5 LED, D7 LED are recommended below, according to the maximum output power of the communications equipment.			
Rated maximum output power of transmitter W	Separation distance according to frequency m		
	150kHz to 80MHz $d=1.2 \times P^{1/2}$	80MHz to 800MHz $d=1.2 \times P^{1/2}$	800MHz to 2,5GHz $d=2.3 \times P^{1/2}$
0,01	0.12	0.12	0.23
0,1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23
For transmitters rated at a maximum output power not listed above, the recommended separation distance $d$ in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where $P$ is the maximum output power rating of the transmitter in watts (W) accordable to the transmitter manufacturer.			
NOTE 1 At 80 MHz and 800 MHz. the separation distance for the higher frequency range applies.			
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			

The device has been tested and homologated in accordance with EN 60601-1-2 for EMC. This does not guarantee in any way that this device will not be effected by electromagnetic interference Avoid using the device in high electromagnetic environment.

## 12. Statement

All rights of modifying the product are reserved to the manufacturer without further notice. The pictures are only for reference. The final interpretation rights belong to GUILIN WOODPECKER MEDICAL INSTRUMENT CO., LTD. The industrial design, inner structure, etc, have claimed for several patents by WOODPECKER, any copy or fake product must take legal responsibilities.



## TABLE OF OPERATING POWER OF THE TIPS

Scaling	
Tip Model	Power
G 1	1-10(G)
G 2	1-10(G)
G 3	1-10(G)
G 4	1-10(G)
G 5	1-10(G)
G 6	1-10(G)
G 7	1-10(G)
G 8	1-10(G)
G 9	1-10(G)
G 10	1-10(G)
G 11	1-10(G)

Periodontics	
Tip Model	Power
P1	1-10(P)
P2L	1-3(P)
P2LD	1-2(P)
P2R	1-3(P)
P2RD	1-2(P)
P3	1-6(P)
P3D	1-6(P)
P4	1-6(P)
P4D	1-6(P)

Endodontics	
Tip Model	Power
E1	1-3(E)
E2	1-3(E)
E3	1-6(E)
E3D	1-3(E)
E4	1-6(E)
E4D	1-3(E)
E5	1-6(E)
E5D	1-3(E)
E8	1-10(E)
E9	1-10(E)
E10	1-6(E)
E10D	1-6(E)
E11	1-6(E)
E11D	1-6(E)
E14	1-3(E)
E15	1-3(E)

Cavity Preparation	
Tip Model	Power
SB1	1-10(P)
SB2	1-10(P)
SB3	1-10(P)
SBL	1-10(P)
SBR	1-10(P)

Scan and Login website  
for more information



Guilin Woodpecker Medical Instrument Co., Ltd.  
Information Industrial Park, Guilin National High-Tech  
Zone, Guilin, Guangxi, 541004 P. R. China

Tel:

Europe Sales Dept.: +86-773-5873196

North/South America & Oceania Sales Dep.: +86-773-5873198

Asia & Africa Sales Dep.: +86-773-5855350 Fax: +86-773-5822450

E-mail: [woodpecker@glwoodpecker.com](mailto:woodpecker@glwoodpecker.com), [sales@glwoodpecker.com](mailto:sales@glwoodpecker.com)

Website: <http://www.glwoodpecker.com>



MedNet EC-Rep GmbH  
Borkstrasse 10 · 48163 Muenster · Germany